

## OPUS

12SXXXXX0



OPUS is the new generation of spectral sensors for online measurement of nitrogen and carbon compounds. Through the analysis of a full spectrum, OPUS is able to deliver reliable readings for  $\text{NO}_3\text{-N}$ ,  $\text{NO}_2\text{-N}$ , organic ingredients ( $\text{COD}_{\text{eq}}$ ,  $\text{BOD}_{\text{eq}}$ ,  $\text{DOC}_{\text{eq}}$ ,  $\text{TOC}_{\text{eq}}$ ), and a number of other parameters.

OPUS features the new TriOS G2 interface, allowing fast and easy configuration of sensors by using

a web browser. Integration into existing process control systems and external data loggers has never been easier.

With the optional battery pack, mobile applications are also feasible. WiFi connectivity allows laptops, tablets or smartphones to be easily used for control without any special application software or app installation.


### Benefits

- Without sampling and preparation of test samples
- Real-time sensor
- Without reagents
- Optical window with nano coating
- Pre-installed application calibration

### Applications

- Sewage treatment plants
- Environmental monitoring
- Drinking water monitoring
- Industrial applications

### Absorption spectrum with/without COD<sub>eq</sub>

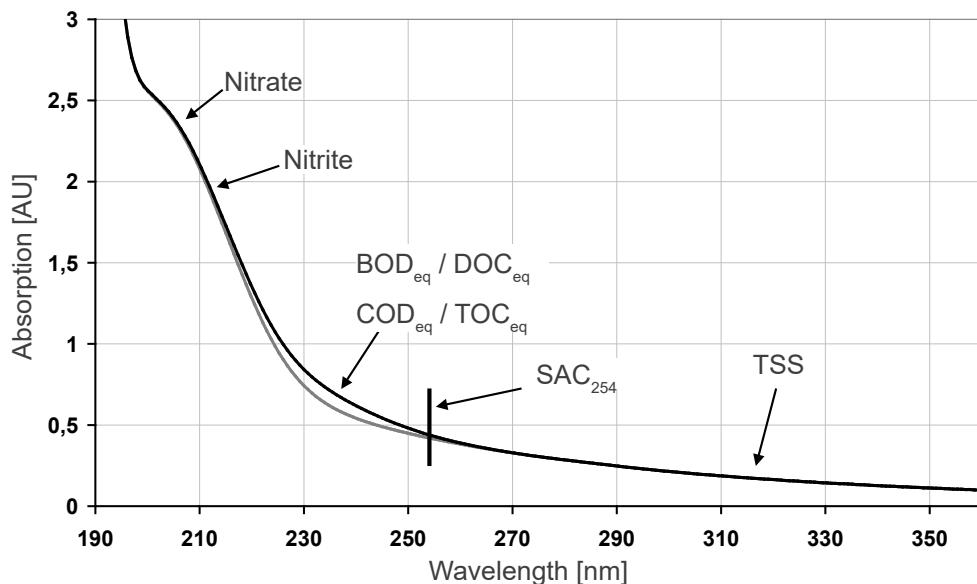

# OPUS

## Technical Specifications

<b>Measure- ment tech- nology</b>	light source  detector	Xenon flash lamp  High-end miniature spectrometer  256 Channels  200 to 360 nm  0.8 nm/pixel	
<b>Measurement principle</b>		Attenuation, spectral analysis	
<b>Optical path</b>		0.3 mm, 1 mm, 2 mm, 5 mm, 10 mm, 50 mm	
<b>Parameter</b>		See parameter list p. 3	
<b>Measuring range</b>		See parameter list p. 3	
<b>Measurement accuracy</b>		See parameter list p. 3	
<b>Turbidity compensation</b>		Yes	
<b>Data logger</b>		~ 2 GB	
<b>T100 response time</b>		2 min	
<b>Measurement interval</b>		≥ 1 min	
<b>Housing material</b>		Stainless steel (1.4571/1.4404), titanium (3.7035), Deep Sea Version: titanium (3.7035)	
<b>Dimensions (L x Ø)</b>		~ 470 mm x 48 mm (10 mm path) Deep Sea Version: ~ 511 x 59 mm	~ 18.5“ x 1.9“ (with 10 mm path) Deep Sea Version: ~ 20.1“ x 2.3“
<b>Weight</b>	stainless steel titanium	~ 3 kg (with 10 mm path) ~ 2 kg Deep Sea Version: ~ 4 kg	~ 6.6 lbs (with 10 mm path) ~ 4.4 lbs Deep Sea Version: ~ 8.8 lbs
<b>Interface</b>	digital	Ethernet (TCP/IP) RS-232 or RS-485 (Modbus RTU)	
<b>Power consumption</b>		≤ 8 W	
<b>Power supply</b>		12...24 VDC (± 10 %)	
<b>Maintenance effort</b>		≤ 0.5 h/month (typical)	
<b>Calibration/maintenance interval</b>		24 months	
<b>System compatibility</b>		Modbus RTU	
<b>Warranty</b>		1 year (EU: 2 years)   US: 2 years	
<b>Max. pressure</b>	with SubConn with fixed cable in FlowCell	30 bar Deep Sea Version: 600 bar 3 bar 1 bar, 2...4 L/min	~ 435 psig Deep Sea Version: ~ 8702.26 psig ~ 43.5 psig ~ 14.5 psig at 0.5 to 1.0 gpm
<b>Protection type</b>		IP68	NEMA 6P
<b>Sample temperature</b>		+2...+40 °C	~ +36 °F to +104 °F
<b>Ambient temperature</b>		+2...+40 °C	~ +36 °F to +104 °F
<b>Storage temperature</b>		-20...+80 °C	~ -4 °F to +176 °F
<b>Inflow velocity</b>		0.1...10 m/s	~ 0.33 fps to 33 fps

# OPUS

## Measuring Range

Single parameter under optimum laboratory conditions

Path (mm)	Parameter	Measurement principle	Unit	Measuring range	Detection limit	Limit of determination	Precision	Accuracy*
1	Nitrate NO <sub>3</sub> -N	Spectral	mg/L	0...100	0.3	0.5	0.05	± (5 % + 0.1)
	Nitrite NO <sub>2</sub> -N	Spectral	mg/L	0...150	0.5	1.2	0.12	± (5 % + 0.1)
	CODeq	Spectral	mg/L	0...2200***	30	100	10	
	BODeq	Spectral	mg/L	0...2200***	30	100	10	
	DOCeQ	Spectral	mg/L	0...1000	5	10	1	
	TOCeq	Spectral	mg/L	0...1000	5	10	1	
	TSSeq	Spectral	mg/L	0...1500	60	200	20	
	KHP	Spectral	mg/L	0...4000	5	10	1	± (5 % + 2)
	SAC <sub>254</sub>	Single wavelength	1/m	0...2200	15	50	5	
	COD-SACeq**	Single wavelength	mg/L	0...3200	22	73	7.3	
	BOD-SACeq**	Single wavelength	mg/L	0...1050	7.2	24	2.4	
10	Nitrate NO <sub>3</sub> -N	Spectral	mg/L	0...10	0.03	0.05	0.005	± (5 % + 0.01)
	Nitrite NO <sub>2</sub> -N	Spectral	mg/L	0...15	0.05	0.12	0.012	± (5 % + 0.01)
	CODeq	Spectral	mg/L	0...220***	3	10	1	
	BODeq	Spectral	mg/L	0...220***	3	10	1	
	DOCeQ	Spectral	mg/L	0...100	0.5	1	0.1	
	TOCeq	Spectral	mg/L	0...100	0.5	1	0.1	
	TSSeq	Spectral	mg/L	0...150	6	20	2	
	KHP	Spectral	mg/L	0...400	0.5	1	0.1	± (5 % + 0.2)
	SAC <sub>254</sub>	Single wavelength	1/m	0...220	1.5	5	0.5	
	COD-SACeq**	Single wavelength	mg/L	0...320	2.2	7.3	0.73	
	BOD-SACeq**	Single wavelength	mg/L	0...105	0.72	2.4	0.24	

\* Based on a standard calibration solution

\*\* Based on KHP (100 mg/L COD standard solution correspond to 85 mg/L KHP)

\*\*\* Depending on composition of COD and BOD (checksum parameter)

1 mg/L NO<sub>3</sub>-N correspond to 4.43 mg/L NO<sub>3</sub>

1 mg/L NO<sub>2</sub>-N correspond to 3.28 mg/L NO<sub>2</sub>



# OPUS

## OPUS G2 Interface

The easiest and fastest way of sensor integration and configuration in any process control system or data logger via web browser:

The figure displays four separate windows of the OPUS G2 software interface:

- MEASUREMENT:** Shows current measurement data for N-NO<sub>3</sub>, TS8eq, System1, CODeq, BODeq, and HA. It includes a spectrum plot, measurement settings (Automatic On, Default Measurement Absorption, Run LSA Yes, Interval 30s, Flash Count 1, Flash Frequency 177, Averaging 1), and buttons for Measure Now!, Measure Absorption!, Measure RAW!, Measure RAW Light!, and Measure RAW Dark!.
- CALIBRATION:** Shows a spectrum plot for a Waterbase sample. It includes calibration settings (Cal Factor 757, Flash Count 1, Lamp Reference 1 757, Lamp Reference 2 356, Temperature Lamp 27.8437 °C, Temperature Spectrometer 25.25 °C) and a Calibrate! button.
- PERIPHERALS:** Shows digital I/O settings for a Transceiver (RS-232, Modbus RTU, 9600 Baudrate, None Flow Control, None Parity, One Stop Bits) and protocol settings (Address 1).
- DIGITAL I/O:** Shows path settings (Path Length 10 mm) and a Save button.

Let OPUS automatically monitor your processes and react to unexpected events or incidents with the optional "policing" feature of OPUS.

